

formerly Aquionics, Berson, Hanovia and Orca GmbH



PURELINE PQ AF

THIRD-PARTY BIOASSAYED UV TREATMENT FOR FOOD & BEVERAGE Our **PureLine PQ AF** systems are aimed specifi ally at providing third party bioassayed UV treatment for product and process waters used in the food and beverage industry.


By using a third-party bioassayed UV system you can be certain that the UV dose being produced will treat the water, eliminate harmful micro-organisms, reduce the bio-burden, protect against bio-fouling, lead to fewer CIP / SIP cycles and lower operating costs.

Each system comes with a certified dry UV sensor allowing checking of UV performance. The UV sensor measures the germicidal output of the UV system and a UV dose read out makes it easy to monitor and log performance.


The control system also has the ability to take fl w and transmittance meter inputs and calculate the UV dose based on real time operating conditions.



POTENTIAL LOCATIONS OF THE PURELINE PQ AF™ IN BOTTLED WATER PROCESSING LINE

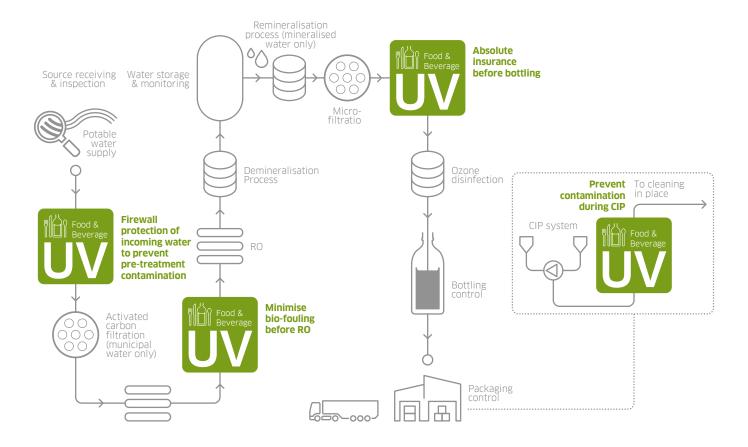

KEY FEATURES	WHAT IT GIVES YOU	BENEFITS FOR YOU		
INTELLIGENCE				
Dry DVGW approved UV sensor measuring germicidal wavelengths	Continuous verification of performance with real time RED dose reading and in-built low dose warning	Easy to monitor and log system performance		
Flow and UV transmittance (UVT) meter inputs	Dose reading based on actual process conditions when meters are connected	Accurate UV dose reading guaranteed under wide range of operating conditions		
OPTIMISATION				
Third party bioassayed UV systems tested in accordance with the USEPA UV Disinfection Guidance Manual	UV system dose equations and sizing have been independently derived	Confidence the system will perform as stated		
UV water treatment	Protect your product and processes from	Does not affect taste and colour of final product		
	microbiological contamination including chlorine resistant Cryptosporidium and Giardia	No chemicals		
	resistant cryptosporiulum and diarulu	Protects pre-treatment equipment and RO filters from bio-fouling, reducing CIP frequency and downtime		
Designed for the food and beverage industry	FDA-approved materials used for all wetted parts	Industry compliant materials		
	*Chamber with tri-clamp connections and < 0.8 µm internal finish	Sanitary design		
	*Automatic wiper (quartz cleaning)	Self cleaning to maintain performance		
INTEGRATION				
Compact design	Can be fitted to skids	Easy integration		
	Can be retrofitted to existing process	_		
RS 485 Modbus * Option	Single cable connection to customer control system			

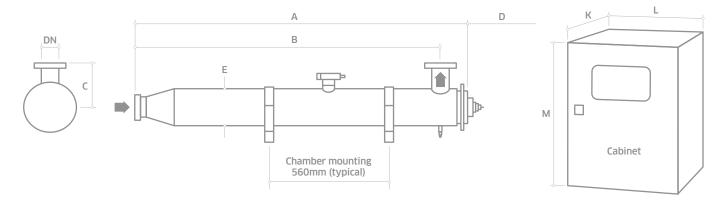

MODEL NUMBER	MAX POWER (W)	MIN T10(%)	DIMENSIONS (MM)				APPROX WEIGHT (KG)						
			Α	В	С	D	Е	DN	К*	L	M**	Chamber (Empty)	Control Cabinet
PureLine PQ AF 0005	125	60	1388	1273	82	1300	102	40	224	600	890	9	36
PureLine PQ AF 0008	200	60	1388	1273	82	1300	102	50	224	600	890	9	36
PureLine PQ AF 0016	350	60	1388	1273	82	1300	102	50	224	600	890	9	36
PureLine PQ AF 0030	350	60	1437	1300	150	1300	168	80	224	600	890	24	36
PureLine PQ AF 0090	750	60	1980	1825	200	1900	206	150	224	600	890	46	36

All dimensions are approximate for clearance purposes only. We have a policy of continuous product development, exact drawings are available on request. All specifications are subject to change without notification. Your distributor or our account manager can advise on correct sizing and specification requirements.

* Allow dimension L in front of cabinet for door opening and panel access.

^{**} M dimension includes the space for the cabinet mounting brackets but you need to allow space below the cabinet for cable entry and access (minimum of 250 mm).

UV CHAMBER	
Material:	StSt 316L / 1.4404
Internal finish:	As made pipe and tube, welds as laid, electropolished and passivated
External finish:	Sateen polish (120 grit) electropolished and passivated
Process (mating) connections:	Flange EN 1092-1 PN16
Drain connection:	Tri-clamp to ISO 2852
End plate:	Removable tri-clamp except PQ AF 0090 which is flanged
Degree of protection:	IP65 equivalent to NEMA 4 but not for outside use
Arc tube (lamp):	Low pressure amalgam
Arc tube enclosure:	Pure quartz (F200)
Number of arc tubes (lamps):	1
Expected lamp life:	12000 hours
Temperature sensor:	Yes
UV sensor:	Dry DVGW compliant UV sensor with UVGuard™ window
Working fluid temperature:	5°C to 40°C
Maximum CIP temperature:	130°C (PQ AF 0005 - PQ AF 0016) 95°C (PQ AF 0030 - PQ AF 0090) with cabinet electrically isolated
Hydrostatically pressure tested:	Yes to PED requirements EN 13445
Chamber mounting:	Horizontal only
Operating pressure:	10 bar (positive pressure only)
Seals:	EPDM, ADI free, EC 1935/2004, FDA 21 CFR 177.2600 approved

21 CFR 177.2600 approved
OPTIONS
Transmittance compensating dose equation
Document Support Pack
Cabinet material: Stainless steel 304
Operation and Maintenance manual and printed Installation and Commissioning manual in Chinese, English, French, German and Spanish
Wiper: Automatic (pneumatically driven)
Flange options: ANSI 150, JIS, Table 'E' and tri-clamp with 0.38 µm internal finish
Chamber internal finish: Tri-clamp chamber only <0.38 µm, welds left as laid, electropolished and passivated
Lead length: 20 & 29 m PQ AF 0005 - 0008, 14 m PQ AF 0016 - 0090
UVShield™
Water leak detection
UL Listing

UL 508A Panel shop

OPTIONS (CONTINUED)
n-field UV reference sensor kit
Max. CIP temperature: 130°C (PQ AF 0030 - 0090, panel switched off)
Welder Document Pack for chamber construction
Bleed: Hygienic valve with tri-clamp connection
Skid mounting (not ship board or earthquake zone)

Material:	Polyester coated carbon steel
Degree of protection:	IP66 / NEMA 4
Supply voltages (nominal):	230 V (+/- 10%) 50/60 Hz
Operating temperature range:	5°C to 40°C
Relative humidity:	<95% non-condensing
Cooling fans:	No
nterconnecting cable lengths:	10 m
ariable power:	Stepless variable power on PQ AF 0090 only (40% reduction from max ballast power, 20% dose reduction)
imi / control	
isplay:	4 line LCD, indicating system

HMI / CONTROL	
Display:	4 line LCD, indicating system status including alarms
Operating menu:	3 levels with password protection
Fault finding:	Event log
CUSTOMER OUTPUTS	
4-20 mA active outputs:	UV dose and UV intensity
24 V dc 10 mA max outputs:	Lamp ON, any trip, any warning, system ready, system in remote, bleed valve

CUSTOMER INPUTS			
4-20 mA active or passive inputs:	Flow meter and transmittance meter		
VFC inputs:	Remote stop/start and remote reset		
CUSTOMER COMMUNICATIONS PORT			

CUSTOMER COM	MUNICATIONS PORT	
RS 485:	Modbus	

APPROVALS

CE marked



PURELINE PQ

Also available in our Food & Beverage product range...



PURELINE DO PURELINE D

PURELINE S

Dechlorination and Chlorine Dioxide removal Ozone removal and treatment

Treatment as part of a multi-barrier approach

Sugar syrup treatment

Canada

+1 980.256.5700 americas@nuvonicuv.com

China

+86 21 61679599 apac@nuvonicuv.com

Germany

+49 611 44575375 emea@nuvonicuv.com

Malaysia

+60 16 440 8834 sea@nuvonicuv.com



Mexico

+1 980.256.5700 americas@nuvonicuv.com

United Kingdom

+44 1753 515300 emea@nuvonicuv.com

USA

+1 980 256 5700 americas@nuvonicuv.com



A Halma company

formerly Aquionics, Berson, Hanovia and Orca GmbH



